





V-Go[®] Product Overview

V-Go[®]: Easy to Use & High Quality Commercial Scale Manufacturing

V-Go Device Overview

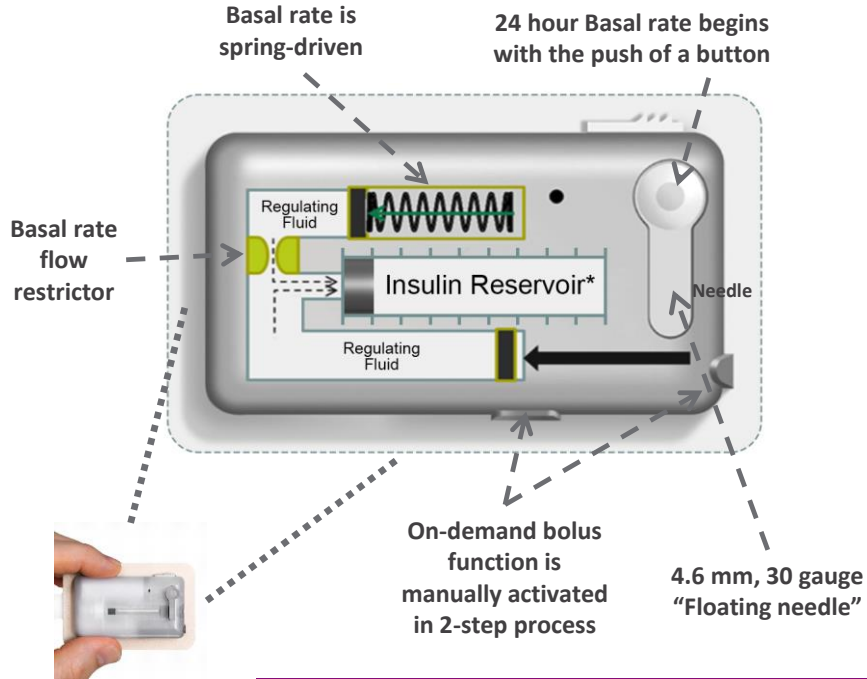

V-Go[®] EZ FILL

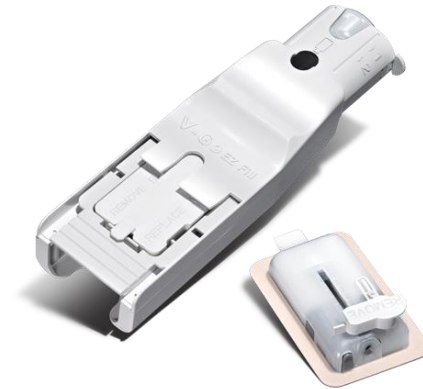


- Simple filling does not require calculations, measuring or needles
- Reduces accidental needle sticks

Robust IP with > 80 patents issued and > 40 pending


Continuous and Consistent Basal Rate

Flow Rate Study of V-Go[®] 30 Units/Day*

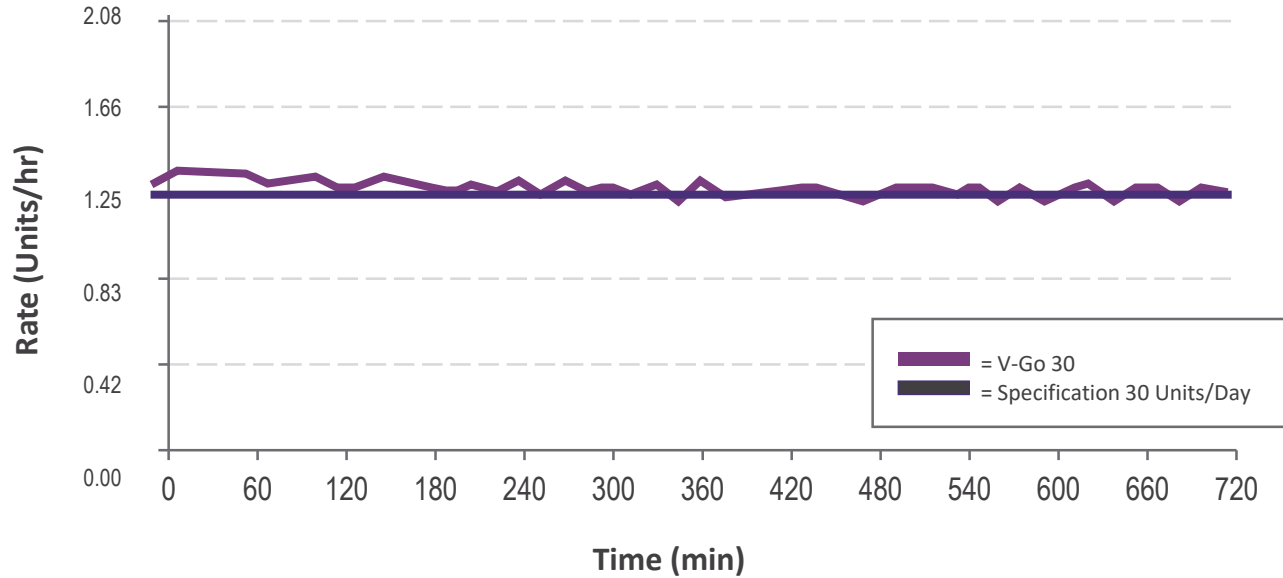


*Proportional results achieved with 20 Units/Day and 40 Units/Day.
Basal and Bolus Accuracy is $\pm 10\%$.

V-Go[®] Combines Simplicity and Physiologic Insulin in Patient-Friendly and Easy-to-Use Wearable Device

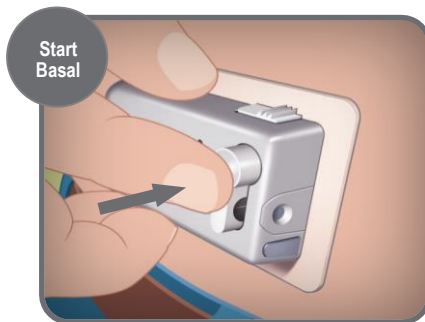

Press button to insert needle and start basal rate of insulin delivered at a constant rate

Deliver on-demand insulin for mealtime coverage in 2 units/click

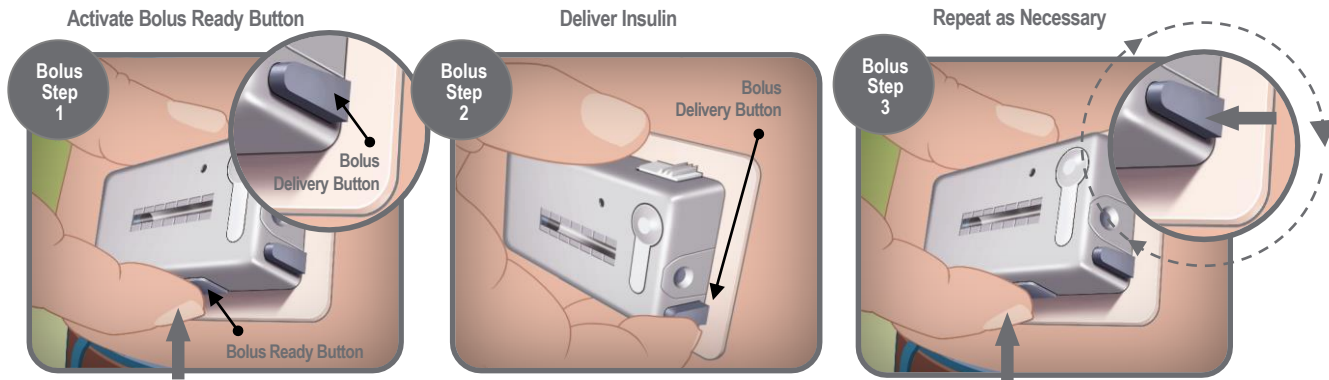

Robust IP with 77 patents issued and 53 pending


Training Patients on V-Go[®]

Fill, Wear & Go...

You, Your Staff, or a Valeritas Representative can easily train the patient



FILL

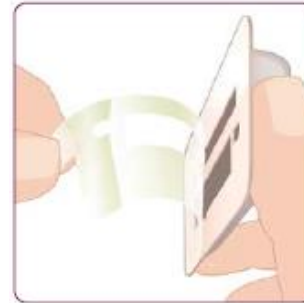




WEAR



GO

V-Go[®] Filling Process

Requires no syringes, measuring or calculating.....

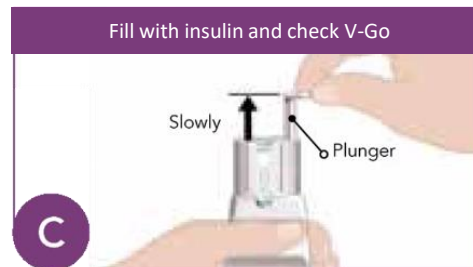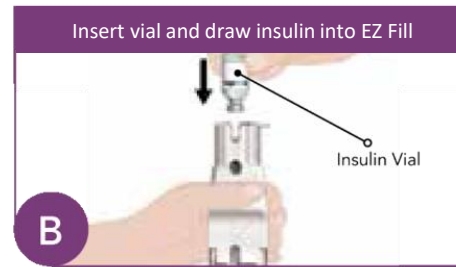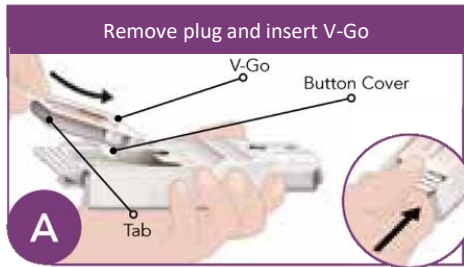

V-Go is filled with a single type of insulin, a U-100 fast-acting insulin (also referred to as a rapid acting insulin). Humalog[®] (insulin lispro, rDNA origin) and NovoLog[®] (insulin aspart, rDNA origin) have been tested by Valeritas and found to be safe for use in V-Go.